

WB-Validated HSPA8 Lentiviral shRNA Knockdown Kit



Catalog #: V61475

Aliases

HSPA8; Heat Shock Protein Family A (Hsp70) Member 8; HSC70; HSP73; HSPA10; HSC71; Lipopolysaccharide-Associated Protein 1; Heat Shock Cognate 71 KDa Protein; Heat Shock 70kDa Protein 8; LPS-Associated Protein 1; LAP-1; Epididymis Secretory Sperm Binding Protein Li 72p; N-Myristoyltransferase Inhibitor Protein 71; Constitutive Heat Shock Protein 70; Epididymis Luminal Protein 33; Heat Shock Cognate Protein 54; Heat Shock 70 KDa Protein 8; Heat Shock 70kd Protein 10; Heat Shock 70kD Protein 8; EC 3.6.4.10; HEL-S-72p; HEL-33; HSC54; HSP71; NIP71; LAP1

Background

Gene Name: HSPA8

NCBI Gene Entry: [3312](#)

Storage

Store at -80 °C for one year.

Kit Components

1. WB-Validated HSPA8 shRNA lentiviral particles (4 mL)
- 2 . Non-Target shRNA lentiviral particles (4 mL)
3. Verification Tool: KD-Validated Anti-Hsc70 Rabbit mAb #61475 (5 µL)

Tested Cell Line

293T

Validation Methods

RT-qPCR; Western Blotting (WB)

Shipping

Shipped with dry ice. Immediately store the product in a standard freezer at -80°C upon receipt.

Instructions For Use

The following protocol uses 293T cell as an example assuming your cell culture medium is DMEM-based.

1.Release 0.5 million 293T cells into a 35 mm tissue culture dish in 2 mL of the growth medium (DMEM containing 10% FBS and 1% pen/strep). Cell density should reach 50-60% confluence the following day.

SUPPORT

SUPPORT@GENUINBIOTECH.COM
TEL: +1-540-855-7041

ORDERS


SALES@GENUINBIOTECH.COM
FAX: +1-540-855-7041

WWW.GENUINBIOTECH.COM

- 2.24 h after cell release, pre-warm the shRNA lentiviral medium to 37°C.
3. Discard 1 mL of the original growth medium of the 35 mm dish.
4. Using a serological pipette, gently mix the lentiviral solution 3 times.
5. Carefully add 1 mL of the lentiviral solution to the well. Tip: To prevent splashing, add the solution to the dish along the wall.
6. Add a polybrene stock solution to the culture medium at a final concentration of 5 µg/mL. Gently swirl the dish to mix.
7. 48 h after cell release, without discarding the original medium, add another 1 mL of lentiviral medium directly into the dish.
8. Add an additional polybrene stock solution into the dish to obtain a final concentration of 5 µg/mL. Tip: Now, the medium in the dish should be a total of 3 mL.
9. 72 h after cell release, cells may reach confluence. Trypsinize the cells off the 35 mm dish and culture those cells in a 60 mm dish.
10. Add puromycin to the dish at a final concentration of 4 µg/mL. Tip: To assess the efficacy of puromycin selection, culture a dish of wild-type 293T cells as a negative control.
11. Allow puromycin selection for 48 h. Almost all wild-type 293T cells should die, while the dish infected with lentiviruses should have some remaining cells.
12. Replace the medium with regular growth medium without puromycin and allow the cells to grow to confluence before harvesting or staining.

Note: 1. This product is for research use only.
2. This product is only supplied to end users.
3. Do not use this product for commercial.


Validation Data

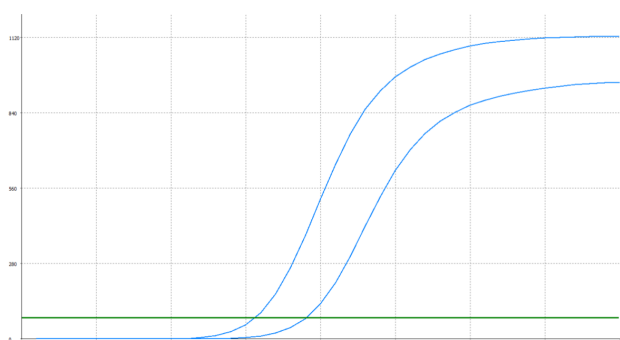

Genotype	Ct Value
Wild-Type	15.61
Knock-Down	18.76
$\Delta Ct (Ct_{KD} - Ct_{WT})$	3.15
% mRNA Reduction	↓ 89%

Copyright ©2024 Genuin Biotechnologies LLC

RT-qPCR analysis. 293T cells were infected with HSPA8-specific shRNA lentiviral particles, total RNA was extracted from wild-type and knockdown cells, RT-qPCR was performed using gene-specific primers. $\Delta Ct (Ct_{KD} - Ct_{WT})$ was used to calculate mRNA reduction (%) between wild-type and knockdown cells using the following formula: $(1 - 1/2^{\Delta Ct}) \times 100\%$.

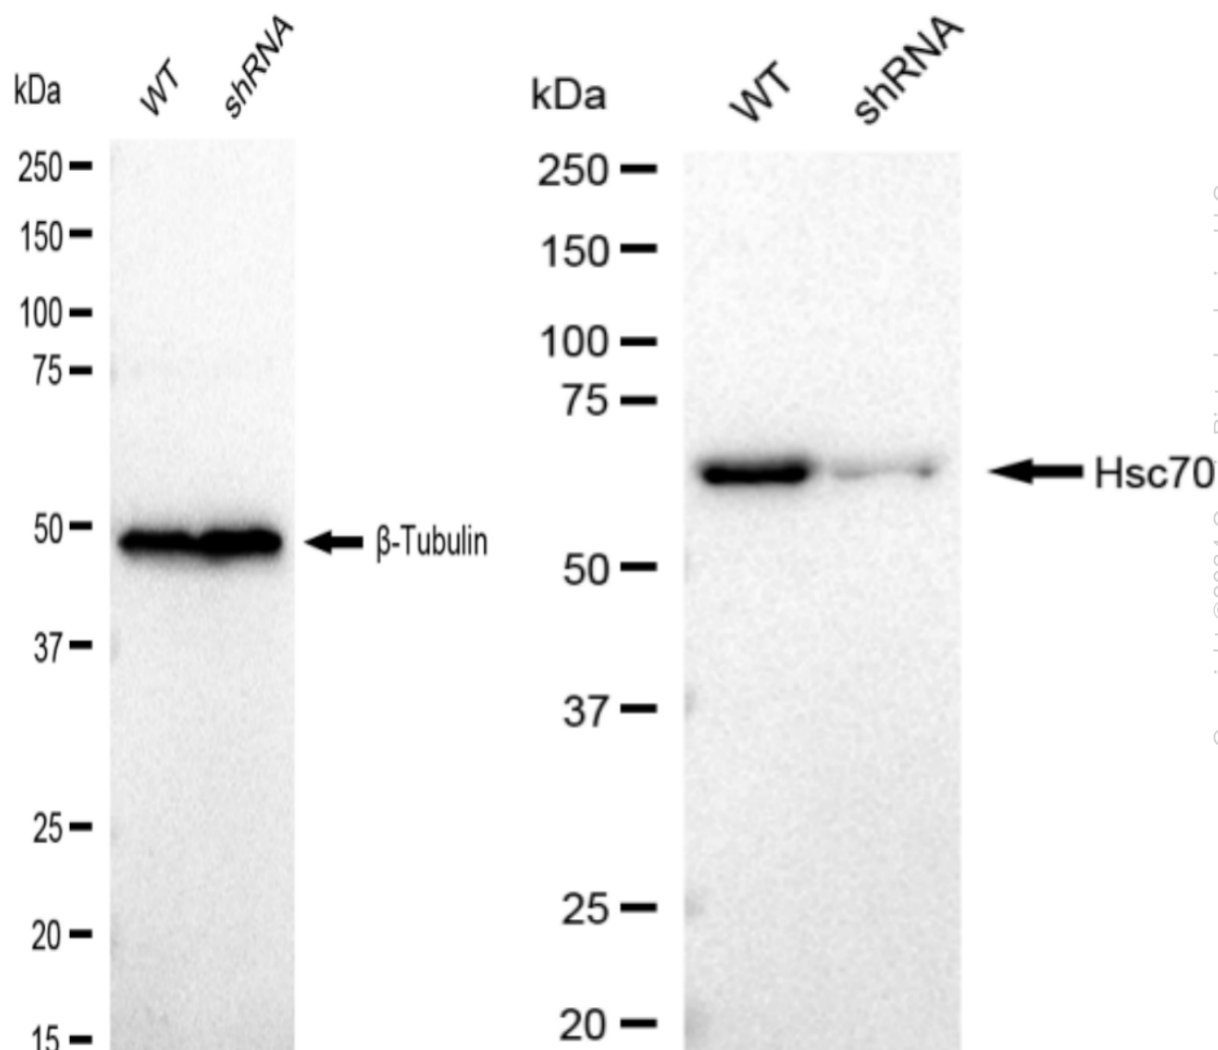

Western blotting analysis. HSPA8 protein expression in wild-type (WT) and shRNA knockdown (KD) 293T cells was detected using Western blotting. β -Tubulin served as a loading control. The blots were incubated with primary antibodies (Cat#61475, 1:5,000) against HSPA8 and β -Tubulin, respectively, followed by incubating with HRP-conjugated goat anti-rabbit secondary antibody (Cat#201, 1:20,000). Images were developed using FeQ™ ECL Substrate Kit (Cat#226).